

NEVER SETTLE. DEBULK THE BEAST!

Remove fibrous tissue swiftly and safely

CUSA® Clarity Ultrasonic Tissue Ablation System
with **Tough Tissue Technology** enables you
to **debulk the toughest tissue**.



INTEGRA[®]
LIMIT UNCERTAINTY

CUSA[®] Clarity
Debulking, Optimized.

Surgeon

Nurse

Administrator

Biomed

NEVER SETTLE Demand CUSA® Clarity Ultrasonic Tissue Ablation System

Enhance Debulking Efficiency With CUSA® TOUGH TISSUE TECHNOLOGY

Only CUSA combines 4 components into 1 integrated system to provide the power and precision you need for quick and safe debulking of fibrous tissue.

TOUGH TISSUE REMOVAL

**160%
FASTER**
vs leading competitor^{1*}




Tough Tissue Tip

BONE REMOVAL

**60%
FASTER**
vs leading competitor^{2†}



Bone Tip

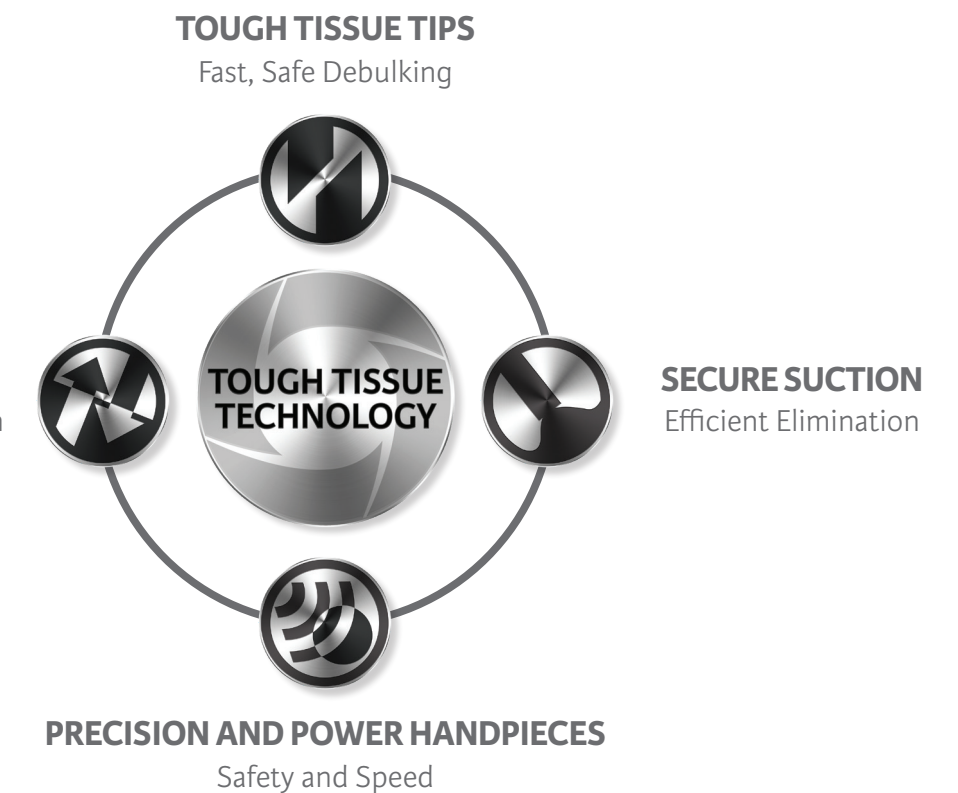


Power Handpiece (23 kHz)

Designed for more challenging neurosurgical procedures including tough tissue and bone removal, as well as other specialties.



Precision Handpiece (36 kHz)

Designed for safety and control in neurosurgical procedures.

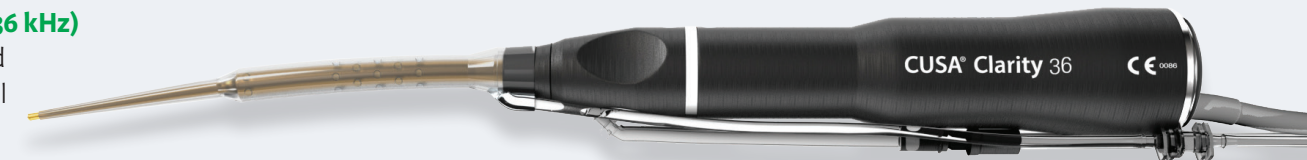

¹On average, with Power Handpiece and Tough Tissue Tip, compared with leading competitor's similar handpiece and tip.
²On average, with Power Handpiece and Bone Tip, compared with leading competitor's similar handpiece and tip.

Optimize Debulking With CUSA® Performance

CUSA Tough Tissue Technology empowers surgical performance



Tough Tissue Technology—the combination of 4 components into 1 integrated system provides the power and precision you need.

CUSA Clarity removes tough tissue 160% faster than the leading competitor.^{1*}



TOUGH TISSUE TIPS

Fast, Safe Debulking

- Power through fibrous tissue quickly and safely via intersecting waves of ultrasonic energy—without sharp cutting edges

Tough Tissue Tip



SECURE SUCTION

Efficient Elimination

- Maintains continuous tissue-tip contact for efficient debulking
- Enabled through strong aspiration—~30% higher than leading competitor[†]




PRECISION AND POWER HANDPIECES

Safety and Speed

- Precision Handpiece (36 kHz) uses high-frequency vibration to localize effect, reducing collateral damage
- Power Handpiece (23 kHz) is designed for more challenging procedures including tough tissue and bone
- Bone removal 60% faster than leading competitor^{1‡}
- Ergonomic design and patent-pending thermal diffusor

Patented Bone Tip

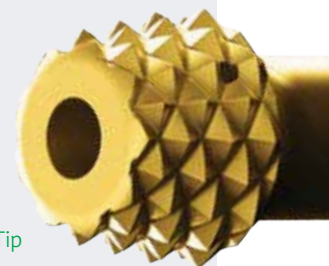

ADAPTIVE POWER

Consistent Fragmentation

- Adjusts power to optimize performance in tough tissue
- Tissue Select® Safety Setting offers additional control around critical structures

^{*}On average, with Power Handpiece and Tough Tissue Tip, compared with leading competitor's similar handpiece and tip.

[†]Based on published specification.

[‡]On average, with Power Handpiece and Bone Tip, compared with leading competitor's similar handpiece and tip.

NEVER SETTLE—DEBULK THE BEAST

With CUSA® Clarity Ultrasonic Tissue Ablation System

- Quick, safe debulking with **Tough Tissue Technology**
- Removes tough tissue 160% faster than leading competitor^{1*}
- Bone removal 60% faster than leading competitor^{1†}
- Precision and Power Handpieces designed for safety, speed, and comfort
- Streamlined setup so CUSA Clarity is ready when you are
- Scalable platform supports future enhancements
- 98.5% Uptime Guarantee with IntegraLink™ Protection Plus¹



Powered by Tough Tissue Technology

*On average, with Power Handpiece and Tough Tissue Tip, compared with leading competitor's similar handpiece and tip.

†On average, with Power Handpiece and Bone Tip, compared with leading competitor's similar handpiece and tip.

Reference: 1. Data on file. Integra LifeSciences. Plainsboro, NJ, USA.

INDICATIONS

The CUSA Clarity Ultrasonic Surgical Aspirator System is indicated for use in surgical procedures where fragmentation, emulsification and aspiration of soft and hard (e.g. bone) tissue is desirable. The CUSA Clarity Ultrasonic Surgical Aspirator is indicated for use in:

Neurosurgery, Plastic and Reconstructive Surgery, Orthopedic Surgery, Gynecological Surgery and Thoracic Surgery and the following specific uses:

Gastrointestinal and Affiliated Organ Surgery—including removal of benign or malignant tumors or other unwanted tissue, including hepatic parenchyma, in open or laparoscopic procedures, hepatic resection, tumor resection, lobectomy or trisegmentectomy, or removal of tissue during liver allotransplantation and donor hepatectomy

Urological Surgery—including removal of renal parenchyma during nephrectomy or partial nephrectomy

General Surgery—including removal of benign or malignant tumors or other unwanted soft or hard tissue in open or minimally invasive general surgical procedures

Laparoscopic Surgery—including removal of hepatic parenchyma in laparoscopic hepatic resection, lobectomy or trisegmentectomy, in laparoscopic donor hepatectomy or laparoscopic cholecystectomy or laparoscopic pancreatic jejunostomy, or pancreatectomy, or laparoscopic appendectomy, laparoscopic colon resection or laparoscopic partial gastrectomy

CONTRAINDICATION

This ultrasonic aspirator device is not indicated for and should not be used for the fragmentation, emulsification, and aspiration of uterine fibroids.

For additional Warnings and Precautions, please see the CUSA Clarity Operator's Manual.

CAUTION: FEDERAL (USA) LAW RESTRICTS THIS DEVICE TO SALE BY OR ON THE ORDER OF A PHYSICIAN. FOR DISTRIBUTION IN THE US ONLY.

CUSA, Tissue Select, Integra, and the Integra logo are registered trademarks of Integra LifeSciences Corporation or its subsidiaries in the United States and/or other countries. IntegraLink is a trademark of Integra LifeSciences Corporation.

For more information or to place an order, please contact:

United States, Canada, Asia, Pacific, Latin America USA 800-654-2873 ■ 888-980-7742 fax Outside USA +1 609-936-5400 ■ +1 609-750-4259 fax integralife.com

©2019 Integra LifeSciences Corporation. All rights reserved. Printed in USA. 1232508-1-EN

Clear and Easy—CUSA® Clarity Ultrasonic Tissue Ablation System


Streamlined to support a smoothly running OR

Ease of Setup

- Guided, step-by-step setup instructions—available right on the touchscreen
- One-step tubing setup with CUSA Quick Connect™ Cartridge and Tubing Set
- On-screen help provides real-time assistance when and where it's needed

Enhanced Reliability and Service

- Handpieces designed for advanced durability
- IntegraLink™ Protection Plus ensures consistent ultrasonic performance and equipment uptime

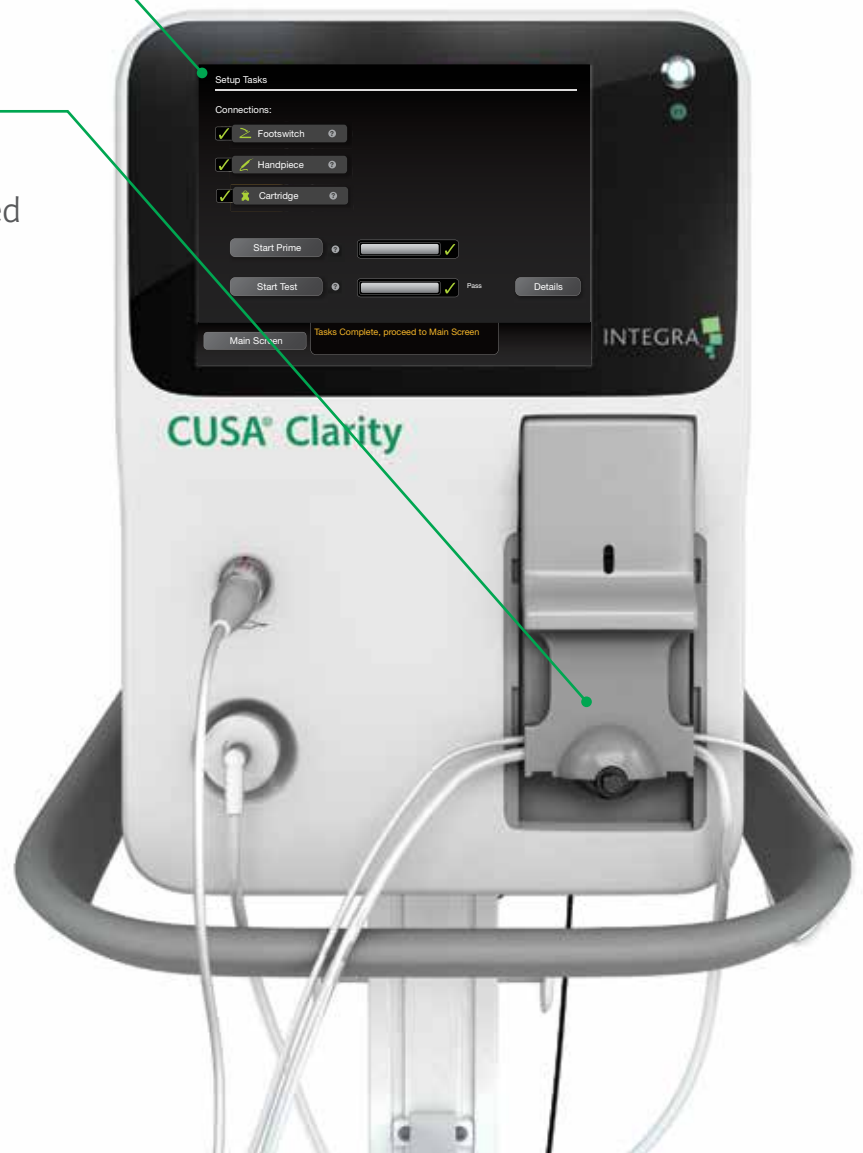

NEVER SETTLE—DEBULK THE BEAST

With CUSA® Clarity Ultrasonic Tissue Ablation System

- Quick, safe debulking with **Tough Tissue Technology**
- Removes tough tissue 160% faster than leading competitor^{1*}
- Bone removal 60% faster than leading competitor^{1†}
- Precision and Power Handpieces designed for safety, speed, and comfort
- Streamlined setup so CUSA Clarity is ready when you are
- Scalable platform supports future enhancements
- 98.5% Uptime Guarantee with Integralink™ Protection Plus¹



Powered by Tough Tissue Technology

*On average, with Power Handpiece and Tough Tissue Tip, compared with leading competitor's similar handpiece and tip.

†On average, with Power Handpiece and Bone Tip, compared with leading competitor's similar handpiece and tip.

Reference: 1. Data on file. Integra LifeSciences. Plainsboro, NJ, USA.

INDICATIONS

The CUSA Clarity Ultrasonic Surgical Aspirator System is indicated for use in surgical procedures where fragmentation, emulsification and aspiration of soft and hard (e.g. bone) tissue is desirable. The CUSA Clarity Ultrasonic Surgical Aspirator is indicated for use in:

Neurosurgery, Plastic and Reconstructive Surgery, Orthopedic Surgery, Gynecological Surgery and Thoracic Surgery and the following specific uses:

Gastrointestinal and Affiliated Organ Surgery—including removal of benign or malignant tumors or other unwanted tissue, including hepatic parenchyma, in open or laparoscopic procedures, hepatic resection, tumor resection, lobectomy or trisegmentectomy, or removal of tissue during liver allotransplantation and donor hepatectomy

Urological Surgery—including removal of renal parenchyma during nephrectomy or partial nephrectomy

General Surgery—including removal of benign or malignant tumors or other unwanted soft or hard tissue in open or minimally invasive general surgical procedures

Laparoscopic Surgery—including removal of hepatic parenchyma in laparoscopic hepatic resection, lobectomy or trisegmentectomy, in laparoscopic donor hepatectomy or laparoscopic cholecystectomy or laparoscopic pancreatic jejunostomy, or pancreatectomy, or laparoscopic appendectomy, laparoscopic colon resection or laparoscopic partial gastrectomy

CONTRAINDICATION

This ultrasonic aspirator device is not indicated for and should not be used for the fragmentation, emulsification, and aspiration of uterine fibroids.

For additional Warnings and Precautions, please see the CUSA Clarity Operator's Manual.

CAUTION: FEDERAL (USA) LAW RESTRICTS THIS DEVICE TO SALE BY OR ON THE ORDER OF A PHYSICIAN. FOR DISTRIBUTION IN THE US ONLY.

CUSA, Integra, and the Integra logo are registered trademarks of Integra LifeSciences Corporation or its subsidiaries in the United States and/or other countries.

CUSA Quick Connect and Integralink are trademarks of Integra LifeSciences Corporation or its subsidiaries.

For more information or to place an order, please contact:

United States, Canada, Asia, Pacific, Latin America USA 800-654-2873 ■ 888-980-7742 fax Outside USA +1 609-936-5400 ■ +1 609-750-4259 fax integrallife.com

©2019 Integra LifeSciences Corporation. All rights reserved. Printed in USA. 1232511-1-EN

CUSA® Clarity Ultrasonic Tissue Ablation System

The clear investment choice

Designed to Help Improve OR Efficiency

- Optimizes fibrous tissue debulking with **Tough Tissue Technology**
- Removes tough tissue 160% faster than the leading competitor^{1*}
- Streamlined setup
- On-screen help provides real-time assistance 24/7 in 20 languages

Investment Protection

- 98.5% Uptime Guarantee with IntegraLink™ Protection Plus, ensuring optimal ultrasonic equipment performance while keeping cost of ownership down¹
- Multispecialty scalable platform supports future enhancements
- Handpieces designed for advanced durability, with patent-pending design

*On average, with Power Handpiece and Tough Tissue Tip, compared with leading competitor's similar handpiece and tip.



NEVER SETTLE—DEBULK THE BEAST

With CUSA® Clarity Ultrasonic Tissue Ablation System

- Quick, safe debulking with **Tough Tissue Technology**
- Removes tough tissue 160% faster than leading competitor^{1*}
- Bone removal 60% faster than leading competitor^{1†}
- Precision and Power Handpieces designed for safety, speed, and comfort
- Streamlined setup so CUSA Clarity is ready when you are
- Scalable platform supports future enhancements
- 98.5% Uptime Guarantee with Integralink™ Protection Plus¹



Powered by Tough Tissue Technology

*On average, with Power Handpiece and Tough Tissue Tip, compared with leading competitor's similar handpiece and tip.

†On average, with Power Handpiece and Bone Tip, compared with leading competitor's similar handpiece and tip.

Reference: 1. Data on file. Integra LifeSciences. Plainsboro, NJ, USA.

INDICATIONS

The CUSA Clarity Ultrasonic Surgical Aspirator System is indicated for use in surgical procedures where fragmentation, emulsification and aspiration of soft and hard (e.g. bone) tissue is desirable. The CUSA Clarity Ultrasonic Surgical Aspirator is indicated for use in:

Neurosurgery, Plastic and Reconstructive Surgery, Orthopedic Surgery, Gynecological Surgery and Thoracic Surgery and the following specific uses:

Gastrointestinal and Affiliated Organ Surgery—including removal of benign or malignant tumors or other unwanted tissue, including hepatic parenchyma, in open or laparoscopic procedures, hepatic resection, tumor resection, lobectomy or trisegmentectomy, or removal of tissue during liver allotransplantation and donor hepatectomy

Urological Surgery—including removal of renal parenchyma during nephrectomy or partial nephrectomy

General Surgery—including removal of benign or malignant tumors or other unwanted soft or hard tissue in open or minimally invasive general surgical procedures

Laparoscopic Surgery—including removal of hepatic parenchyma in laparoscopic hepatic resection, lobectomy or trisegmentectomy, in laparoscopic donor hepatectomy or laparoscopic cholecystectomy or laparoscopic pancreatic jejunostomy, or pancreatectomy, or laparoscopic appendectomy, laparoscopic colon resection or laparoscopic partial gastrectomy

CONTRAINDICATION

This ultrasonic aspirator device is not indicated for and should not be used for the fragmentation, emulsification, and aspiration of uterine fibroids.

For additional Warnings and Precautions, please see the CUSA Clarity Operator's Manual.

CAUTION: FEDERAL (USA) LAW RESTRICTS THIS DEVICE TO SALE BY OR ON THE ORDER OF A PHYSICIAN. FOR DISTRIBUTION IN THE US ONLY.

CUSA, Integra, and the Integra logo are registered trademarks of Integra LifeSciences Corporation or its subsidiaries in the United States and/or other countries. Integralink is a trademark of Integra LifeSciences Corporation.

For more information or to place an order, please contact:

United States, Canada, Asia, Pacific, Latin America USA 800-654-2873 ■ 888-980-7742 fax Outside USA +1 609-936-5400 ■ +1 609-750-4259 fax integrallife.com

©2019 Integra LifeSciences Corporation. All rights reserved. Printed in USA. 1232515-1-EN

IntegraLink™ Protection Plus— What a Service Partnership Should Be

Equipment Optimization and Performance

- New replacement handpieces due to accidental misuse*—up to 2 per year
- Software updates to support future enhancements
- 98.5% Uptime Guarantee to minimize equipment downtime and OR disruptions¹

Investment Protection and Uptime Guarantee

- Guaranteed value—up to 2 NEW handpieces at the end of the contract period[†]
- 24-hour guaranteed shipment of all handpieces
- On-site annual preventive maintenance
- Online training and certification for Biomed Staff

*Applies to both Precision and Power Handpieces.

[†]Based on the purchase of 1 console and 2 handpieces—choice of Precision and/or Power Handpieces (36kHz or 23kHz), assuming 2 replacement handpieces were not already provided during the agreement for misuse.



NEVER SETTLE—DEBULK THE BEAST

With CUSA® Clarity Ultrasonic Tissue Ablation System

- Quick, safe debulking with **Tough Tissue Technology**
- Removes tough tissue 160% faster than leading competitor^{1*}
- Bone removal 60% faster than leading competitor^{1†}
- Precision and Power Handpieces designed for safety, speed, and comfort
- Streamlined setup so CUSA Clarity is ready when you are
- Scalable platform supports future enhancements
- 98.5% Uptime Guarantee with Integralink™ Protection Plus¹



Powered by Tough Tissue Technology

*On average, with Power Handpiece and Tough Tissue Tip, compared with leading competitor's similar handpiece and tip.

†On average, with Power Handpiece and Bone Tip, compared with leading competitor's similar handpiece and tip.

Reference: 1. Data on file. Integra LifeSciences. Plainsboro, NJ, USA.

INDICATIONS

The CUSA Clarity Ultrasonic Surgical Aspirator System is indicated for use in surgical procedures where fragmentation, emulsification and aspiration of soft and hard (e.g. bone) tissue is desirable. The CUSA Clarity Ultrasonic Surgical Aspirator is indicated for use in:

Neurosurgery, Plastic and Reconstructive Surgery, Orthopedic Surgery, Gynecological Surgery and Thoracic Surgery and the following specific uses:

Gastrointestinal and Affiliated Organ Surgery—including removal of benign or malignant tumors or other unwanted tissue, including hepatic parenchyma, in open or laparoscopic procedures, hepatic resection, tumor resection, lobectomy or trisegmentectomy, or removal of tissue during liver allotransplantation and donor hepatectomy

Urological Surgery—including removal of renal parenchyma during nephrectomy or partial nephrectomy

General Surgery—including removal of benign or malignant tumors or other unwanted soft or hard tissue in open or minimally invasive general surgical procedures

Laparoscopic Surgery—including removal of hepatic parenchyma in laparoscopic hepatic resection, lobectomy or trisegmentectomy, in laparoscopic donor hepatectomy or laparoscopic cholecystectomy or laparoscopic pancreatic jejunostomy, or pancreatectomy, or laparoscopic appendectomy, laparoscopic colon resection or laparoscopic partial gastrectomy

CONTRAINDICATION

This ultrasonic aspirator device is not indicated for and should not be used for the fragmentation, emulsification, and aspiration of uterine fibroids.

For additional Warnings and Precautions, please see the CUSA Clarity Operator's Manual.

CAUTION: FEDERAL (USA) LAW RESTRICTS THIS DEVICE TO SALE BY OR ON THE ORDER OF A PHYSICIAN. FOR DISTRIBUTION IN THE US ONLY.

CUSA, Integra, and the Integra logo are registered trademarks of Integra LifeSciences Corporation or its subsidiaries in the United States and/or other countries. Integralink is a trademark of Integra LifeSciences Corporation.

For more information or to place an order, please contact:

United States, Canada, Asia, Pacific, Latin America USA 800-654-2873 ■ 888-980-7742 fax Outside USA +1 609-936-5400 ■ +1 609-750-4259 fax integrallife.com

©2019 Integra LifeSciences Corporation. All rights reserved. Printed in USA. 1232518-1-EN

NEVER SETTLE—DEBULK THE BEAST

With CUSA® Clarity Ultrasonic Tissue Ablation System

- Quick, safe debulking with **Tough Tissue Technology**
- Removes tough tissue 160% faster than leading competitor^{1*}
- Bone removal 60% faster than leading competitor^{1†}
- Precision and Power Handpieces designed for safety, speed, and comfort
- Streamlined setup so CUSA Clarity is ready when you are
- Scalable platform supports future enhancements
- 98.5% Uptime Guarantee with IntegraLink™ Protection Plus¹



Powered by Tough Tissue Technology

*On average, with Power Handpiece and Tough Tissue Tip, compared with leading competitor's similar handpiece and tip.
†On average, with Power Handpiece and Bone Tip, compared with leading competitor's similar handpiece and tip.

Reference: 1. Data on file. Integra LifeSciences. Plainsboro, NJ, USA.

INDICATIONS

The CUSA Clarity Ultrasonic Surgical Aspirator System is indicated for use in surgical procedures where fragmentation, emulsification and aspiration of soft and hard (e.g. bone) tissue is desirable. The CUSA Clarity Ultrasonic Surgical Aspirator is indicated for use in:

Neurosurgery, Plastic and Reconstructive Surgery, Orthopedic Surgery, Gynecological Surgery and Thoracic Surgery and the following specific uses:

Gastrointestinal and Affiliated Organ Surgery—including removal of benign or malignant tumors or other unwanted tissue, including hepatic parenchyma, in open or laparoscopic procedures, hepatic resection, tumor resection, lobectomy or trisegmentectomy, or removal of tissue during liver allotransplantation and donor hepatectomy

Urological Surgery—including removal of renal parenchyma during nephrectomy or partial nephrectomy

General Surgery—including removal of benign or malignant tumors or other unwanted soft or hard tissue in open or minimally invasive general surgical procedures

Laparoscopic Surgery—including removal of hepatic parenchyma in laparoscopic hepatic resection, lobectomy or trisegmentectomy, in laparoscopic donor hepatectomy or laparoscopic cholecystectomy or laparoscopic pancreatic jejunostomy, or pancreatectomy, or laparoscopic appendectomy, laparoscopic colon resection or laparoscopic partial gastrectomy

CONTRAINDICATION

This ultrasonic aspirator device is not indicated for and should not be used for the fragmentation, emulsification, and aspiration of uterine fibroids.

For additional Warnings and Precautions, please see the CUSA Clarity Operator's Manual.

CAUTION: FEDERAL (USA) LAW RESTRICTS THIS DEVICE TO SALE BY OR ON THE ORDER OF A PHYSICIAN. FOR DISTRIBUTION IN THE US ONLY.

CUSA, Integra, and the Integra logo are registered trademarks of Integra LifeSciences Corporation or its subsidiaries in the United States and/or other countries. IntegraLink is a trademark of Integra LifeSciences Corporation.

For more information or to place an order, please contact:

United States, Canada, Asia, Pacific, Latin America USA 800-654-2873 ■ 888-980-7742 fax Outside USA +1 609-936-5400 ■ +1 609-750-4259 fax integrallife.com

©2019 Integra LifeSciences Corporation. All rights reserved. Printed in USA. 1195179-2-EN



CUSA® Clarity

Debulking, Optimized.